CARDIOCADDY

Cabinet Installation Guide

Included with your cabinet


- ✓ 4 x M6 expansion bolts, to fix the cabinet to a wall
- ✓ 4 x M6 penny washers, to use inside the cabinet
- ✓ Entry code
- ✓ 2 x Cabinet side stickers
- ✓ Cabinet User Guide

Electrical Information

- > This cabinet meets Class II double insulation standards
- > The heater is rated 50W (note: a brief, yet high, inrush current occurs for approx. 0.5 sec.)
- The LED strip is rated 3W
- Hardwire the cabinet to a 3A fused spur.

Mounting the cabinet to a building

- Risk asses your install location.
 Choose a site where the cabinet will not take drainage (e.g. water dripping from a roof) and ideally, a site which avoids the cabinet being in direct sunlight for extended periods of time.
- 2. Remove cabinet from packaging.
- 3. Measure and mark the four fixing hole locations (W:340mm, H:275mm), ensuring the **bottom** of the cabinet is approximately 1.1m up off the ground.
- 4. Measure the mid-point between the 2 lower holes, then measure 50mm vertically up and mark. This is for the power cable hole. Offer up cabinet to check alignment.

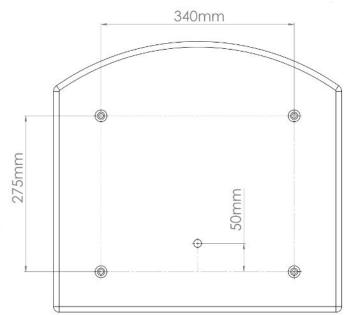


- 5. Drill out the four fixing holes, using an appropriate 12mm drill bit.
 - a. Clear dust and debris from holes.
- 6. Drill out the power cable hole angle the hole slightly uphill to prevent water ingress.
- 7. Insert the anchors and tighten the bolts to expand and secure the sleeves.
- Now unscrew the bolts, offer up the cabinet, and attach using the same bolts along with the M6 penny washers.
 Do not over-tighten as this may distort the cabinet if the mounting surface is not flat use resin mounted bolts and spacers if necessary.
- 9. Run the power cable through the wall.
- A competent person should hard wire the cabinet to a fused spur, with isolation switch (use an all-pole disconnecting device, with contact gap of at least 3mm in the switched off state). The feed to the cabinet should also be protected by a Residual Current Device (RCD).

Final Checks

- > Once there is power to the cabinet, the internal light will come on and the heater will be ready
- > The heater is pre-set to automatically switch on at ~8C and switch off at ~15C
- Fit the two Heart Restarter stickers onto the sides of the cabinet (if desired). Align them with the smooth areas, to ensure good adhesion
- There is an Information Sticker inside the cabinet with maintenance instructions, electrical information and the cabinet serial number.

If you have any queries, please contact your cabinet supplier.









CARDIOCADDY