ARTMASTER 453564695051 REV II



1 TURN ON

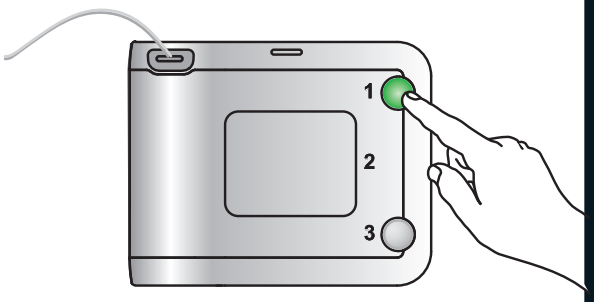

2 Bare chest.
Clean and dry if needed.

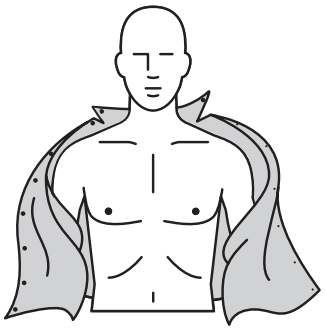

3 Open gray pads case.

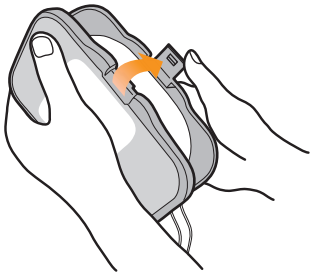

4 Peel each pad.

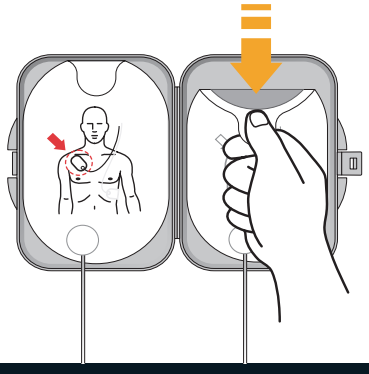

5 Place pads on chest.

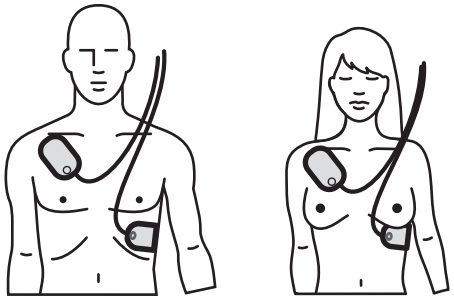

6 Analyzing . . . Stand back

WAIT UNTIL  STOPS FLASHING

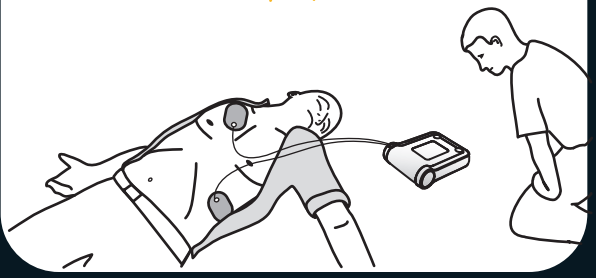

7 Press flashing orange shock button.

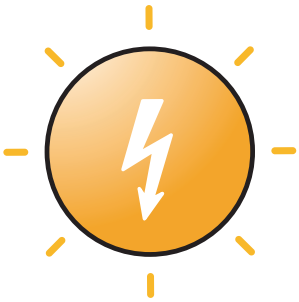

8 For CPR help: Press the flashing blue button.





INFANT/CHILD

< 55 lbs / 25 kg (0-8 years)



INFANT/CHILD

Insert key at beginning of rescue.

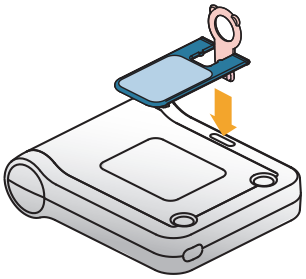

Place pads on back and chest.

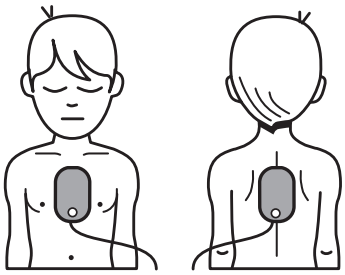

Philips Medical Systems
22100 Bothell Everett Highway
Bothell, WA 98021-8431, USA

EC REP Philips Medizin Systeme Boeblingen GmbH
Hewlett-Packard Str. 2
71034 Boeblingen, Germany

Copyright © 2017 Koninklijke Philips N.V.

MADE IN USA

453564695051 REV II

CE 0123 ℞ ONLY

REF 989803138601

453564695051

PHILIPS